




Hotplate, acid resistant CP300

Instructions for use
Manuel d'utilisation
Istruzioni per l'uso
Instrucciones de
funcionamiento
Bedienungsanweisung

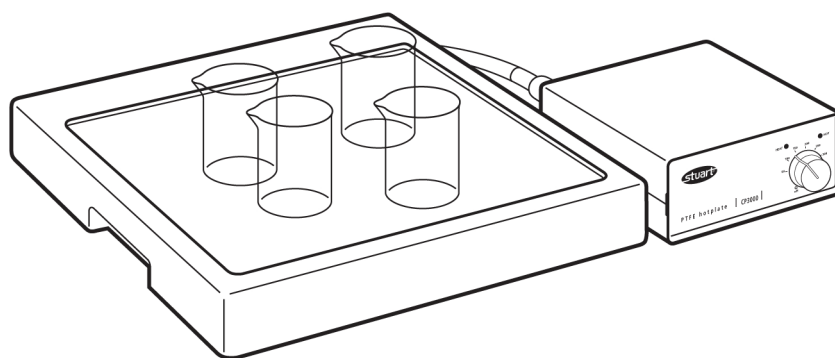

Hotplate

CP300

Instructions for use

Introduction

Thank you for purchasing this piece of Stuart equipment. To get the best performance from the equipment and for your own safety, please read these instructions carefully before use. Before discarding the packaging check that all parts are present and correct.

This equipment is designed to operate under the following conditions:

- ❖ For indoor use only
- ❖ Use in a well ventilated area
- ❖ Ambient temperature range +5°C to +40°C
- ❖ Altitude to 2000m
- ❖ Relative humidity not exceeding 80%
- ❖ Mains supply fluctuation not exceeding 10%
- ❖ Over-voltage category II IEC60364-4-443
- ❖ Pollution degree 2
- ❖ Use with a minimum distance all around of 200mm from walls or other items

If the equipment is not used in the manner described in this manual and with accessories other than those recommended by Stuart, the protection provided may be impaired.

Electrical Installation



THIS EQUIPMENT MUST BE EARTHED

Before connection please ensure that the line supply corresponds to that shown on the rating plate.

Model	Supply requirements
CP300	230V, 50 or 60Hz,~, single phase

The unit is supplied with two mains leads fitted with IEC plugs for connection to the control box. One has a U.K. 3 pin plug and the other has a 2 pin "Shuko" plug for connection to the mains. Choose the lead appropriate for your electrical installation and discard the other. Should neither lead be suitable, take the lead with the U.K. plug and replace the plug with a suitable alternative. This involves cutting off the moulded plug,

preparing the cable and connecting to the re-wireable plug in accordance with its instructions.

THIS OPERATION SHOULD ONLY BE UNDERTAKEN BY A QUALIFIED ELECTRICIAN

The wires in the mains cable are coloured as follows:

BROWN	-	LIVE
BLUE	-	NEUTRAL
GREEN/YELLOW	-	EARTH

The control unit is fitted with an IEC socket at the rear for connection of the mains lead.

The appropriate mains lead should be connected **BEFORE** connection to the mains supply.

Should the mains lead need replacement, a cable of 1mm² of harmonised code H05W-F connected to an IEC320 plug should be used.

NOTE: Refer to the equipment's rating plate to ensure that the plug and fusing are suitable for the voltage and wattage stated. The UK mains lead is protected by a 10A fuse mounted in the plug top.

Model	Power	Fuse
CP300	900W	T5A

Fuse fitted in both live and neutral lines.

IF IN DOUBT CONSULT A QUALIFIED ELECTRICIAN

Safety Advice Before Use


- ❖ Do not use to heat flammable materials.
- ❖ Position the instrument on a firm level surface away from any heat sensitive or flammable material.
- ❖ Never move or carry the unit while it is in use or connected to the mains supply. Switch off and allow to cool for at least 30 minutes.
- ❖ The unit should be carried using both hands with fingers under each side frame.
- ❖ In the case of mains interruption, a fault or failure, the unit **WILL** continue to operate on removal of the fault.
- ❖ **NEVER** immerse the hotplate unit in acid or any other liquid. The unit has breather holes in the base which will allow liquid access that will destroy sensitive components.

General Description


The acid resistant hotplate consists of a ceramic tile and heater assembly mounted in a block of high grade PTFE. The hotplate is controlled via a separate control unit which is connected by a 2 metre lead (partly covered with a PTFE sleeve). This allows the hotplate to be located in a fume hood and the controller outside, away from the corrosive environment.

Controls

Front of control unit

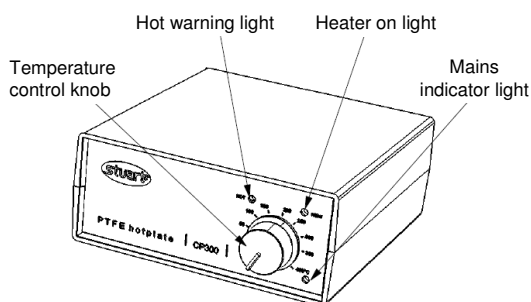

Rear of control unit

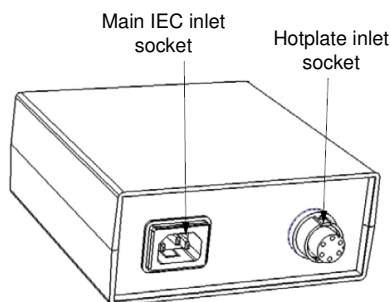

Operation

1. Position the hotplate unit on a firm level surface away from any heat sensitive or flammable material.
2. Plug the hotplate lead into the hotplate inlet socket of the control unit.
3. Connect the control unit to the mains supply (the green mains indicator light will illuminate).
4. Position the control unit in the area it is to be used (e.g. outside the fume hood).
5. Turn the control unit ON using the temperature control knob and select the temperature of the hotplate by using the printed scale around the knob. The heater on light will illuminate.

6. When the hotplate surface is hot (>50°C) the hot warning light will begin to flash red. This will continue to flash while the plate temperature is above 50°C even after the hotplate has been switched off (the control unit must remain connected to the mains supply).

Maintenance



WARNING: Before attempting to clean the unit, ensure that the hotplate is cool and that the control unit is disconnected from the mains electricity supply.

The control unit should be cleaned using a damp cloth and mild detergent solution. Do not use harsh or abrasive cleaning agents.

The hotplate body can be cleaned with almost any cleaning agent compatible with PTFE. A damp cloth will remove most types of contamination. For more difficult stains a domestic cleaner is recommended.

Cleaning is made easier if spillages are attended to promptly. In any case, spillages of alkali, phosphoric acid and hydrofluoric acid **MUST** be removed immediately as these chemicals can attack and damage the glass ceramic. Ensure the appropriate safety precautions are observed.

NEVER immerse the hotplate unit in acid or any other liquid. The unit has breather holes in the base which will allow liquid access that will destroy sensitive components.

WARNING: A ceramic top which is scratched, chipped, chemically etched or damaged must not be used.

Servicing

This product does not require any routine servicing.

NOTE: There are no internal user-replaceable parts.

In the event of a product failure any repairs or replacement of parts MUST only be undertaken by suitably qualified personnel.

For advice, please contact the Service Department, quoting both the model number and serial number:

E-mail: service@bibby-scientific.com

Tel: +44 (0)1785 810475
Fax: +44 (0)1785 810471

Only spare parts supplied or specified by Stuart or its agents should be used. Fitting of non-approved parts may affect the performance of the safety features designed into the instrument. If in any doubt, please contact the Service Department of Bibby Scientific Ltd. or the point of sale.

For any other technical enquiries, please contact the Technical Support Department:
E-mail: stuarthelp@bibby-scientific.com,
Tel: +44 (0)1785 810433.

Warranty

Stuart warrants this equipment to be free from defects in material and workmanship, when used under normal laboratory conditions, for a period of **three (3)** years. In the event of a justified claim, Stuart will replace any defective component or replace the unit free of charge.

This warranty does NOT apply if damage is caused by fire, accident, misuse, neglect, incorrect adjustment or repair, damage caused by installation, adaptation, modification, fitting of non-approved parts or repair by unauthorised personnel.

This warranty does NOT apply if the ceramic top has broken due to mechanical impact, scratching, chipping or chemical etching.

Bibby Scientific Ltd.
Beacon Road,
Stone, Staffordshire
ST15 0SA
United Kingdom
Tel: +44 (0) 1785 812121
Fax: +44 (0) 1785 813748
E-mail: equipment@bibby-scientific.com
www.stuart-equipment.com

Technical Specification

	CP300
Plate material (hotplate)	Glass ceramic
Body material (hotplate)	PTFE
Plate dimensions	300 x 300mm
Heated area	200 x 200mm
Heater power	900W
Maximum plate temperature	400°C
Hotplate dimensions (w x d x h)	320 x 360 x 60mm
Control unit dimensions (w x d x h)	150 x 160 x 65mm
Lead length	2m
Net weight	11kg
Electrical supply	230V, 50-60Hz



This product meets the relevant EC harmonised standards for radio frequency interference and may be expected not to interfere with, or be affected by, other equipment with similar qualifications. We cannot be sure that other equipment used in its vicinity will meet these standards and we cannot guarantee that interference will not occur in practice. Where there is a possibility that injury, damage or loss might occur if equipment malfunctions due to radio frequency interference, or for general advice before use, please contact the Technical Service Department of Bibby Scientific Ltd.

Declaration of Conformity

PTFE Hotplate, Model CP300

These products comply with the requirements of the EU Directives listed below:

2004/108/EC **EMC Directive.**
2006/95/EC **Low voltage Directive (LVD)**


Compliance with the requirements of these Directives is claimed by meeting the following standards:

EN 61326-1:2006 (Electrical Equipment for Measurement, Control and Laboratory use).
EN 61010-1: 2001
(Safety Requirements Electrical Equipment for Measurement, Control and Laboratory use)
EN 61010-2-010: 2003 (Particular Requirements for Laboratory Equipment for Heating of Materials).

The technical documentation required to demonstrate that the product meets the requirements of these standards is available for inspection upon request.

Reference Reports: 120101TR(EMC), 120201TR(LVD).

CE mark affixed '03.

Signed:  (Mr C. Warren)

Date: JUNE 2009

Authority: Technical Manager
Bibby Scientific Ltd



Bibby Scientific Ltd - Stone - Staffs - ST15 0SA - UK
Tel: +44 (0) 1785 812121 - Fax +44 (0) 1785 813748

INSPECTION REPORT

MODEL **CP300**


ELECTRICAL SAFETY

- 1. Earth continuity
- 2. Insulation
- 3. Flash test

FUNCTIONAL

- 1. Indicators
- 2. Heating function
- 3. Visual acceptance

QUALITY CONTROL INSPECTOR



UK

Bibby Scientific Ltd.
Beacon Road,
Stone
Staffordshire,
ST15 0SA
UK
Tel: +44 (0)1785 812121
Fax: +44 (0)1785 810405
E-mail: sales@bibby-scientific.com
www.bibby-scientific.com

France

Bibby Scientific Limited
Bâtiment Le Deltaparc Parc
Silic PN2
7 rue du Canal
BP 55437 VILLEPINTE
95944 ROISSY Charles de
Gaulle
France
Tel: +33(0)148 63 78 03
Fax: +33(0)148 63 78 01
E-mail: ventes@bibby-scientific.com
www.bibby-scientific.com

North and South America

Bibby Scientific US Inc. t/a
Techne Inc.
3 Terri Lane, Suite 10
Burlington, N.J. 08016 USA
Toll Free (in NA): 800-225-9243
Tel: +1 609 589 2560
Fax: +1 609 589 2571
E-mail:
labproducts@techneusa.com
www.techneusa.com

Italy

Bibby Scientific Italia Srl
Via Alcide de Gasperi 56
20070 Riozzo di Cerro al
Lambro (MI)
Italia
Tel: +39 (0)2 98230679
Fax: +39 (0)2 98230211
E-mail: marketing@bibby-scientific.it
www.bibby-scientific.it

Middle East

Bibby Scientific Middle East Ltd.
PO Box 27887, Engomi 2433
Nicosia
Cyprus
Tel: +357 22 660 423
Fax: +357 22 660 424
E-mail: sales@bibby-scientificme.com

Asia

Bibby Scientific - Singapore
Prudential Tower, Level 26
30 Cecil Street
Singapore 049712
Tel: +65 6631 2976
Fax: +44 (0) 1785 810405
E-mail: info@bibby-scientific.com
www.bibby-scientific.com